




SAS-Chicago

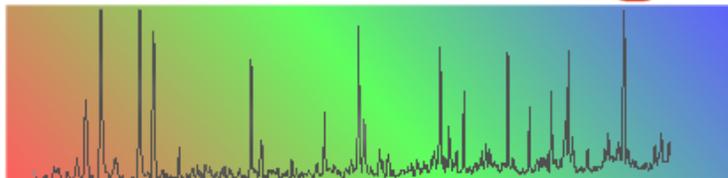

Please visit our linked business cards on the [last page](#) of this flyer.

November Meeting

Tuesday, November 9, 2004

The November 2004 meeting will be held at the LaMirage Restaurant, located at 3223 Algonquin Rd., Rolling Meadows. See the map on the following page.

Social Hour: 5:30 - 6:30 PM

Dinner: 6:30 PM

Speakers: 7:45 – 9:00 PM

Student Night

Presentations by

Northwestern and NIU Graduate Students

- Chanda Ranjit Yonzon; Northwestern University - fourth year graduate student working under Professor Richard P. Van Duyne

Topic: Surface-Enhanced Raman Scattering Based Glucose Sensor

- John Carr; Northern Illinois University - third year graduate student working under Dr. Jon Carnahan

Topic: Effects of Various Liquid Chromatography Mobile Phase Solvent Compositions and Buffers for Pharmaceutical Nonmetal Detection with ICP-AES and ICP-MS

- Kaho Kwok; Northern Illinois University - third year graduate working under Dr. Jon Carnahan

Topic: HPLC Separation of Pharmaceutical Compounds with ICP-MS Detection

- Matt Young; Northwestern University – third year graduate student working under Professor Richard P. Van Duyne and Professor Peter Stair

Topic: Wavelength-Scanned Surface-Enhanced Raman Excitation Spectroscopy on Well-Defined Silver Nanoparticle Arrays

Please make your dinner reservations for the upcoming meeting by using the form on our web page < <http://www.sas-chicago.org/Online%20Registration.htm> >, by email at sas.chicago@bigfoot.com or by calling Mary Kaplar at 708-449-5767. Leave **your name, company affiliation, a telephone number, the number of reservations and your choice of entree**. Please call by **noon Friday, Nov. 5th**, so that proper arrangements can be made with the LaMirage Restaurant. If you can't attend, cancel by Mon. noon: SAS is charged for no-shows.

Entree choices: NY Strip Steak, Chicken Breast LaMirage, or Fettuccini.

Dinner Cost Members: \$25

Students: Free

Unemployed Members: \$10

Non-members: \$30

Surface-Enhanced Raman Scattering Based Glucose Sensor

According to World Health Organization, 150 million people in the world suffer from diabetes. Diabetic patients require frequent glucose measurements and careful control of glucose levels for the long-term health outlook. Numerous studies have been performed toward developing a real-time, quantitative, and biocompatible glucose sensor. This work presents a surface-enhanced Raman scattering (SERS) based glucose sensor. Ethylene glycol-terminated alkanethiol is self-assembled on a silver film over nanosphere to partition glucose within the zone of electromagnetic field enhancement. Glucose concentration is quantitatively predicted using a Chemometric method and presented in the industry standard Clarke error grid. Moreover, stability, reusability, and biocompatibility of this glucose sensor will be discussed.

Effects of Various Liquid Chromatography Mobile Phase Solvent Compositions and Buffers for Pharmaceutical Nonmetal Detection with ICP-AES and ICP-MS

Detection of heteroatoms such as sulfur, phosphorous, chlorine and fluorine is finding increasing importance in the pharmaceutical industry. Pharmaceutical compounds and their associated impurities may be separated and detected using either high performance liquid chromatography or ion chromatography. Classical detectors such as UV or mass spectrometry typically require a set of standards for each analyte to obtain accurate results as detectors responses vary for analytes of different structures. Plasmas are a potentially excellent atom reservoir for atomic spectrometry. Inductively coupled plasma atomic emission spectrometry (ICP-AES) and inductively coupled plasma mass spectrometry (ICP-MS) has the potential to effectively atomize the analyte allowing element specific detection while eliminating the need for standards. However, plasma systems typically produce somewhat higher nonmetal detection limits due to the decreased ionization and excitation efficiencies of these elements. Additionally, various LC mobile phase compositions and gradients are utilized in the separation process. The composition of the solution can have an effect on the analytical response. Efforts to examine and alleviate the aforementioned problems are examined utilizing membrane desolvation techniques. A comprehensive study of the effects of various mobile phase compositions and buffers on the signal intensity of phosphomycin, a biologically active, phosphorous containing analyte is presented. Optimization conditions and results for both ICP-AES and ICP-MS will be presented. Comparisons of detection limits obtained for both instruments as well as signal response using various mobile phases will be highlighted.

HPLC Separation of Pharmaceutical Compounds with ICP-MS Detection


High performance liquid chromatography (HPLC) has become a technique of choice for analytical separations of pharmaceutical compounds. Throughout the years, detection techniques for HPLC such as UV absorption, refractive index, and mass spectrometry have become common. However, there are drawbacks in these detection techniques. For instance, since the response of these detectors usually varies with the chemical structure of the compound of interest, internal standards are required for each analyte in order to obtain accurate quantitative results. Because inductively coupled plasma mass spectrometry (ICP-MS) rely on sample decomposition to convert analytes to atomic forms, such drawbacks can be minimized or eliminated. Sensitivity and selectivity can be enhanced by using ICP-MS as detector for pharmaceutical separations with HPLC. The analytical performance of our ICP-MS for non-metals (P, S, Cl, and F) detection will be presented. The performance of an HPLC system with ICP-MS detection for the separation of several pharmaceutical compounds containing non-metals will be presented. The ability to quantify impurities in these compounds with HPLC-ICP-MS will be discussed.

Wavelength-Scanned Surface-Enhanced Raman Excitation Spectroscopy on Well-Defined Silver Nanoparticle Arrays

This work presents the most thorough wavelength-scanned excitation spectroscopy study to date. Ag nanoparticles, fabricated using nanosphere lithography, are used as substrates, providing extremely well-characterized and size-homogenous nanoparticle arrays. Surface-enhanced Raman scattering (SERS) intensities of adsorbed benzenethiol monolayers are correlated to the localized surface plasmon resonance (LSPR) of the nanoparticle arrays. SER spectra are taken using excitation wavelengths from 425-800 nm and a triple spectrograph. The SER excitation spectra are shown to have similar lineshapes to the LSPR spectra. In addition, the maximum SERS enhancement is shown to occur for wavelengths slightly shorter than the excitation wavelength such that both the incident photon and the Raman scattered photon are strongly enhanced. Three different Raman peaks of benzenethiol are studied simultaneously on one substrate and it is shown that the smaller Raman shifted peak shows a maximum enhancement closer to the LSPR λ_{\max} than that of a larger Raman shifted peak. This is in qualitative agreement with what is predicted by the electromagnetic enhancement mechanism. Enhancement factors of up to 1×10^8 are achieved, which is in good agreement with previous SERS studies done on these substrates.

DIRECTIONS TO THE LA MIRAGE RESTAURANT

[LaMirage](#) is located at 3223 Algonquin Road in Rolling Meadows. It is located about 0.5 mile east of Route 53 on Algonquin Road. The LaMirage restaurant is on the south side of the road.



Index of Newsletter Sponsors

(Click on card or URL to link to Sponsor's web site)


5225 Verona Road
Madison, WI
53711-4495

Andrew M. Haefner, Ph.D.
Sales Engineer
Molecular Spectroscopy

(800) 648-5456
(815) 479-0127 fax
(815) 479 0887 direct

andrew.haefner@thermo.com www.thermo.com

www.thermo.com

[email](mailto:andrew.haefner@thermo.com)



➤ **Steve Bouffard, Ph.D.**
Technical Sales Specialist
FTIR, UV/Vis/NIR, GC, GC/MS
HPLC, DSC, TGA, TMA and DMA

➤ **PerkinElmer Life and Analytical Science**
2000 York Road, Suite 132
Oak Brook, IL 60523
Phone: (800) 762-4000
Fax: (203) 944-4914
Steven.Bouffard@perkinelmer.com
www.perkinelmer.com

www.perkinelmer.com

[email](mailto:Steven.Bouffard@perkinelmer.com)


'Tools for Discoveries of Life'

Rina K. Dukor, Ph.D.
President / CEO

Tel: (847) 487-5500
Fax: (847) 487-5544
Toll Free: (866) BTOOLS1
E-mail: rkdukor@btools.com
Website: www.btools.com

Bio Tools, Inc.
950 N. Rand Rd. Unit 123
Wauconda, IL 60084 USA

www.btools.com

[email](mailto:rkdukor@btools.com)

JERRY SHKOLNIK
Executive Sales Representative
Chicago, IL


TELEDYNE INSTRUMENTS
Leeman Labs
A Teledyne Technologies Company

6 Wentworth Drive
Hudson, New Hampshire 03051
Phone: 847.478.0452 Fax: 847.478.0467
Toll Free: 1.800.634.9942 Cell: 603.493.6176
E-Mail: JShkolnik@Teledyne.com
www.LeemanLabs.com

www.leemanlabs.com

[email](mailto:JShkolnik@Teledyne.com)



➤ **Jeff Kukuk**
Senior Sales Engineer
Inorganic Analysis

➤ PerkinElmer, Inc.
2000 York Road, Suite 132
Oak Brook, IL 60523
Phone: 800 762-4000 ext. 132
Fax: 630 556-4523
Cell: 630 222-8921
jeff.kukuk@perkinelmer.com
www.perkinelmer.com

www.perkinelmer.com

[email](mailto:jeff.kukuk@perkinelmer.com)

Chip McCauslin
Sales Representative-Atomic Spectroscopy
Analytical Chemist
Chicago Area
Optical Spectroscopy Instruments


VARIAN

Varian Analytical Instruments
2700 Mitchell Drive
Walnut Creek, CA 94598
Phone: 800.926.3000 Ext. 3025
Fax: 925.945.2360
http://www.varianinc.com
chip.mccauslin@varianinc.com

www.varianinc.com

[email](mailto:chip.mccauslin@varianinc.com)



For the best in nebulizers, sample introduction components, torches, and spray chambers, call:
1-800-MEINHARD

Meinhard Glass Products
Geoff Coleman, Ph.D., Vice President

700 Corporate Circle, Suite A
Golden, Colorado 80401-5636 USA
Tel: 303.277.9776 Fax: 303.216.2649
gcoleman@meinhard.com www.meinhard.com

www.meinhard.com

[email](mailto:gcoleman@meinhard.com)



Contact Mary Kaplar to get your business card in the next SAS-Chicago section newsletter.

makaplar@yahoo.com

[email](mailto:makaplar@yahoo.com)